Device type	SVAN 971	
Serial No.	84012	
Pre Calibration type	By measurement	
Pre Calibration date	2-7-2022	
Pre Calibration time	21:53:12	
Post Calibration type	By measurement	
Post Calibration date	3-7-2022	
Post Calibration time	01:35:46	
Pre Calibration factor	1.3 dB	
Pre Calibration level	94.0 dB	
Post Calibration factor	1.4 dB	
Post Calibration level	94.0 dB	
Calibration drift	-0.1 dB	

1S413.SVL : Logger results

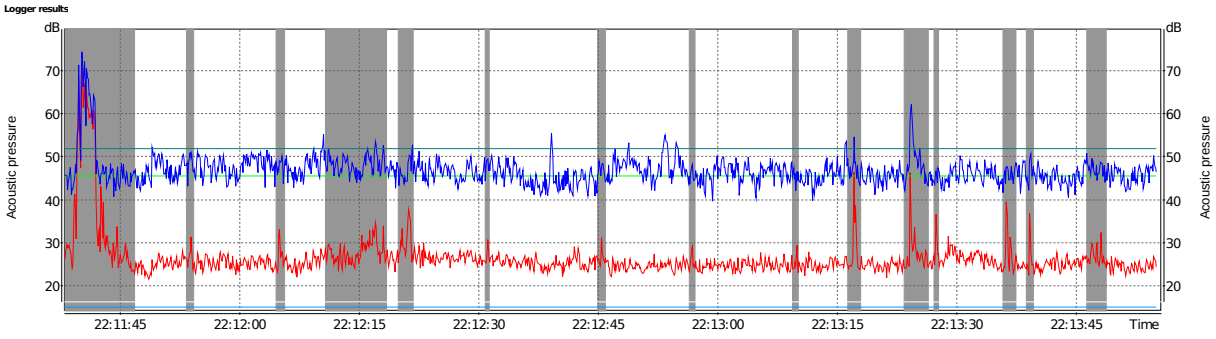

	Start	Duration	LAeq (TH) [dB] P1 (A, Lin)	LAeq (SR) [dB] P1 (A, Lin)	LCeq (TH) [dB] P2 (C, Lin)	LCeq (SR) [dB] P2 (C, Lin)
Info	-	-				
Main cursor	02-07-2022 22:13:55.000	-	24.3	45.5	46.5	51.8
Inside blocks	02-07-2022 22:11:38.100	00:00:33.100	51.7	45.5	56.7	51.8
Outside blocks	02-07-2022 22:11:38.000	00:01:43.900	25.4	45.5	47.0	51.8
Events	02-07-2022 22:11:38.000	00:02:17.000	-	-	-	-

1S414.SVL : Logger results, zoom out = 3x (max envelope)

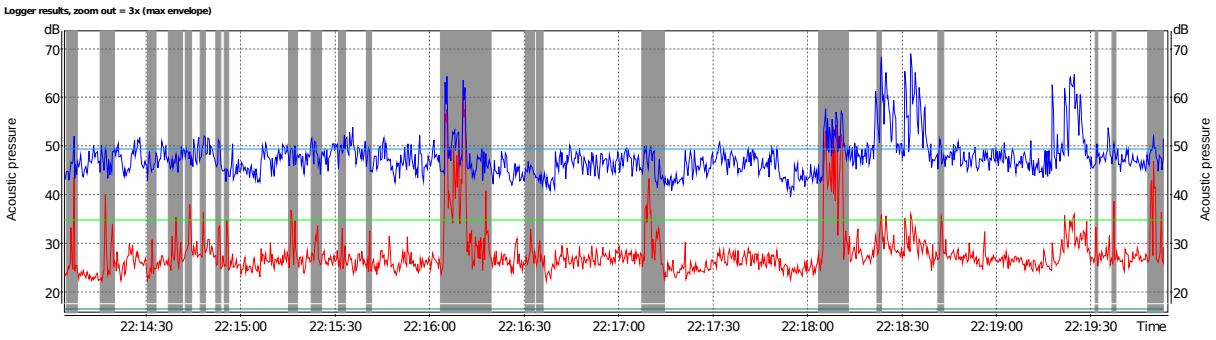

	Start	Duration	LAeq (TH) [dB] P1 (A, Lin)	LAeq (SR) [dB] P1 (A, Lin)	LCeq (TH) [dB] P2 (C, Lin)	LCeq (SR) [dB] P2 (C, Lin)
Info	-	-				
Main cursor	02-07-2022 22:19:53.000	-	max:29.3	max:34.8	max:51.5	max:49.4
Inside blocks	02-07-2022 22:14:04.600	00:01:20.800	40.7	34.8	49.8	49.4
Outside blocks	02-07-2022 22:14:04.000	00:04:28.200	26.4	34.8	49.3	49.4
Events	02-07-2022 22:14:04.000	00:05:49.000	-	-	-	-